KR2000/3000 SERIES with measured **GRAPHIC RECORDER**



KR2000/3000 series are paperless recorders that prevent falsification of data to meet the requirements of FDA 21CFR Part11 for medicinal chemical manufacturing. Employs high visibility display and high operating function. Also it realize data recording and management by easy operation.

*FDA 21CFR Part 11: The U.S. Food and Drug Administration rule on electronic records and electronic signatures. It is a requirement when replacing the paper-based records to electronic media and enacted in 1997.



data protection

KR2000 144 x 144 mm Size 5.6" TFT color LCD Display




KR3000 288 x 288 mm Size 12.1" TFT color LCD Display

FEATURES

Easy operation Touch screen (KR3000) High speed sampling 100ms

Export data to USB flash drive LAN network capability

Various functions such as calculation

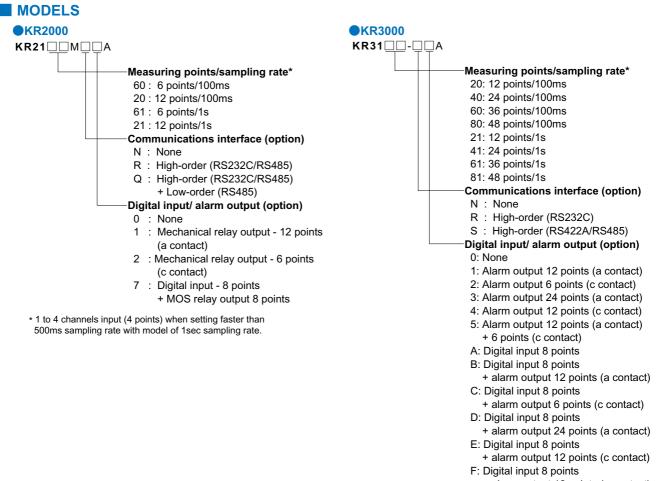


+ alarm output 12 points (a contact) + alarm output 6 points (c contact)

PREVENTING FALSIFICATION OF DATA

Store the file in binary format. Display a message if falsified.

Binary file example


* Example when opened by word pad.



AUDIT TRAIL

Electronic signature to electronic record file. Display audit operation.

Audit trail screen

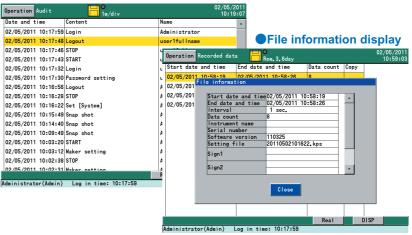

LOGIN FUNCTION

Register up to 5 administrators and 100 general users and only registered users can access. Set 10 kinds of access authority and signature level.

Login user registration

0p	eration Real tr	end	Rem. 3. 1day				02	/05/2011 10:14:39	utho	ority & sig	nat	ire level						
	ID		Full name		Authori	ty	Passwor					02/05/2011	-					
1	USER1	•	user1fuliname	•	1	•	Clear	Operation Real to	rend	e 1sec		02/05/2011 10:15:47	OLog	gin scro	een			
2	GUEST1	•	guest1hullname	•	2	*	Clear	Authority 1	- Auth	nority name Atrn1	-	Operation	Paul Au		● Rem. 3. 8day		(02/05/2011 09:58:20
3		-		•	1	•	Clear									0.00		
4		-		-	1	•	Clear	Alarm ACK	9	Delete file	9		00 2 00 8	0.00 3	0.00 4	0.00 5	0.00 6	0.00
5		-		•	1	•	Clear					-10		-5	0.00	0.00	5	10
6		•		٠	1	×	Clear	START/STOP	R	Copy file		Signature 2		l	🔫 .		1 yr ran y	
7		•		•	1	•	Clear	MENU/HOME settings	R	FTP transfer		Signature 3		Login				
8		•		-	1			DISP menu	R	Delete marker	R	Signature 4	_	ID	Admin	•		
9		-		-	1	•	Clear	Set clock	R	Write marker	2							
10	1	-		•	1	•	Clear											
11		•		٠	1	•	Clear						_	Password		•		
12		-		•	1	•	Clear											
	Return													Login	ר	Cancel		
Adm	inistrator(Admi	n)	.og in time: 10:00:42	-	_	-	_											
, ruin		., .						Return										
								Administrator(Admi	n) Lo	og in time: 10:00:4	12							
										-						Hist	DISP	

Smooth Operation by touch screen!

KR3000 SERIES

Input / Computation setting

Easy setting and display

Operation Real trend	Rem. 3. 4day	02/05/2 10:01
CH. 1	Copy from 1 - to 1 - Go	
Range type 10V 🔹		
Range -10,00 -	to 10.00 -	
Scale		
Correction 10.00		
RJ t	INS DEL BS Set Cancel	
Burn out		
Tag 0 1 2	2 3 4 5 6 7 8 9	
Unit V +	E	
Calculate OFF		
Formula	•	
Return		
Administrator(Admin) Log	in time: 10:00:42	

Login operation

Easy-to-input the letter and value by touching.

ID Admin	•
Password	•
Login	Cancel

ation	Real	trend	1)© 1sec							02/05, 10:0
ABC	ab		INS	DEL	в	s	Set	Can	cel			
A	В	,	D	E	F	,	н		J	к	L	м
N	0	Ρ	Q	R	s	т	U	v	W	х	Y	z
0	1	2	3	4	5	6	7	8	9	<u> </u>		
+	-	*	1	%	^	()	•	-	:	;	<
_	=	!	{	}	\mathbf{N}			_				



Data replay, CSV conversion

ZAILA-P Exclusive application software (standard attached)


By using exclusive application software, each file can data replay, confirm audit trail, signature, print, convert to PDF and convert to CSV file.

Each file recorded in KR2000 & KR 3000 can be taken out by USB flash drive.

KR3000







INPUT SPECIFICATIONS

Measuring points:	KR2000 6 points, 12 points
	KR3000 12 points, 24 points, 36 points, 48 points
Input types:	Universal (refer to the table of measuring range)
Accuracy ratings:	0.1% digit (exceptions) * Measurement range conversion
	accuracy
Reference junctior	n compensation accuracy:
	K, E, J, T, N, Platinel 2 0.5 or less
Sampling rate:	100ms Approximately 100ms for all points
	1 ms Approximately 300ms for all points*
Burnout:	Disconnection of input signal is detected on thermocouple
	and resistance input.

* When sampling rate is set below 0.5s at KR2P61/ KR2P21, then input will automatically becomes 4 points and sampling rate will be 100ms.

RECORDING SPECIFICATIONS

Internal memory:	512MB
Exterior memory:	Store the data file to USB flash drive
Recording cycle:	100, 200, 500ms, 1, 2, 3, 5, 10, 15, 20, 30s
	1, 2, 3, 5, 10, 15, 20, 30, 60min
Logging data:	Measured data Time of day, month and year of recording
	start, tag, measured data, alarm status/types, maker text,
	etc
	Setting parameter All setting parameter
	Computation result data
Store types:	Binary type
Storing methods:	Manual start / stop
	Schedule (designation for time of day and date)
	Trigger signal (alarm event, digital input)
	Data logging of before and after trigger points
* Pre-trigger is sel	ectable

Measuring numbers of pre-trigger --- Max 950 data

COMPUTATION SPECIFICATIONS

Computation points:

KR2000	Maximum 44 points
KR3000	Maximum 128 points

Computation types:

Arithmetic operation, comparison operations, logical operations, integration operations, channel data operations, dew point, relative humidity, wind direction, 16 direction display, increment per time, remaining amount of internal memory, abnormality judgment, user lockout judgment

DISPLAY SPECIFICATIONS

Display types:

Measured data display (Trend screen, Data screen, Bar-graph screen) Historical trend display (Simultaneous display with Real-time trend is available) Information display (alarm display, marker list, file list, audit trail) Setting screen KR2000 --- Max 44 points KR3000 --- Max 56 points Display points:

*The LCD display may contain some pixels that always or never illuminate, and the brightness of some areas of the display may appear uneven. There are typical LCD performance characteristics and do not constitute malfunctions.

COMMUNICATION SPECIFICATIONS Network

unication С

Communication	Communication type.							
	Ethernet (10BASE-T/100BASE-TX)							
FTP client:	Transfer a data file to a network server							
SNTP client:	The time can be synchronized to the time of SNTP server							
E-Mail:	E-Mail notification at specified time for alarm activation							
	Report data at specified time is selectable from all							
	registered data							
	Notification address Maximum 8 contacts							

ALARM SPECIFICATIONS

Setups:	Up to 4 alarms can be programmed per channel
Alarm types:	Upper limit, lower limit, differential upper limit, differential
	lower limit (deadband is selectable), abnormal data
Delay function:	Setup range of alarm delay 0 to 3600 seconds
Alarm settings:	AND/OR selectable

GENERAL SPECIFICATIONS

Rated power volta	age:
	100 to 240V AC (universal power supply) 50/60Hz
Maximum power	consumption:
	KR2000 50VA
	KR3000 65VA
Normal operating	condition:
	Ambient temperature & humidity 0 to 50°C, 20 to 80%RH
	Power voltage 90 to 264V AC
	Power frequency 50/60Hz±2%
	Attitude left/right/forward tilting 0°C, backward tilting 0 to
	20%
Weight:	KR2000 About 2.2kg (max)
	KR3000 About 7.2kg (max)
Mounting:	Panel mounting

STANDARDS

Protection:	KR2000 IEC529 IP65 compliance (front part)
	KR3000 IEC529 IP54 compliance (front part)
CE:	KR2000 (approved)
	KR3000 (approved)
	EMC directive EN61326-1 Class A
	EN61000-3-2
	EN61000-3-3
	Low voltage directive EN61010-1
	Over voltage (installation) category II, pollution level 2,
	measuring category II
*The indication	aquivalant to 1mV may vary under the test anvironment by

he indication equivalent to 1mV may vary under the test environment by **EMC** directives

OPTION SPECIFICATIONS

Please see standard version's PS sheets.



MEASURING RANGES

					Acouroourotingo
	Input type	-13.80	to	ng range 13.80mV	Accuracy ratings
	DC voltage	-13.80 -27.60 -69.00 -200.0 -500.0 -2.000	to to to to to to	27.60mV 69.00mV 200.0mV 500.0mV 2.000V	±0.1%±1digit
 \	(with built-in roltage divider)	-5.000 -10.00 -20.00 -50.00	to to to to	5.000V 10.00V 20.00V 50.00V	
	к	-200.0 -200.0 -200	to to to	300.0℃ 600.0℃ 1370℃	
	E	-200.0 -200.0 -200	to to to	200.0℃ 350.0℃ 900℃	±0.1%±1digit *-200 to 0°C:
	J	-200.0 -200.0 -200	to to to	250.0℃ 500.0℃ 1200℃	±0.2%±1digit
	Т	-200.0 -200.0	to to	250.0°C 400.0°C	
	R	0	to to	1200°C 1760°C	±0.1%±1digit *0 to 400°C:
	S	0 0	to to	1300°C 1760°C	±0.2%±1digit
	В	0	to	1820°C	±0.1%±1digit *0 to 400°C:Out of accuracy ratings *400 to 800°C: 0.15%±1digit
	Ν	-200.0 -200.0 -200	to to to	400.0℃ 750.0℃ 1300℃	±0.15%±1digit *-200 to 0°C : ±0.3%±1digit
T/C	W-WRe26	0	to	2315℃	±0.15%±1digit *0 to 100°C: ±4%±1digit *100 to 400°C: ±0.5%±1digit
	WRe5-WRe26	0	to	2315℃	±0.2%±1digit
	PtRh40-PtRh20	0	to	1888℃	±0.2%±1digit *0 to 300°C: ±1.5%±1digit *300 to 800°C: ±0.8%±1digit
	NiMo-Ni	-50.0 -50.0 -50	to to to	290.0°C 600.0°C 1310°C	±0.2%±1digit
	CR-AuFe	0.0	to	280.0K	±0.2%±1digit *0 to 20K: ±0.5%±1digit *20 to 50K: ±0.3%±1digit
	Platinel II	0.0 0.0 0	to to to	350.0°C 650.0°C 1395°C	±0.15%±1digit
	U	-200.0 -200.0 -200.0	to to to	250.0℃ 500.0℃ 600.0℃	±0.15%±1digit *-200 to 0°C: ±0.3%±1digit
	L	-200.0 -200.0 -200	to to to	250.0℃ 500.0℃ 900℃	±0.1%±1digit *—200 to 0°C : ±0.2%±1digit
	Pt100	-140.0 -200.0 -200.0	to to to	150.0℃ 300.0℃ 850.0℃	±0.1%±1digit *-140.0 to 150.0°C 700 to 850°C: ±0.15%±1digit
RTD	JPt100	-140.0 -200.0 -200.0	to to to	150.0℃ 300.0℃ 649.0℃	±0.1%±1digit *-140.0 to 150.0°C : ±0.15%±1digit
	Pt50	-200.0	to	649.0°C	±0.1%±1digit
	Pt-Co	4.0	to	374.0K	±0.15%±1digit *4 to 50K : ±0.3%±1digit


The accuracy ratings are converted into the measuring range under reference operatingcondition. Thermocouple input does not contain reference junction compensation accuracy. K.E.J.T.R.S.B.N : IEC584,JIS C1602-1995 W-WRe26,WRe26,PIRh40-PIRh20,PlatineIII,NiMo-Ni,Cr-AuFe : ASTM Vol14.03 U(Cu-CuN),IL(Fe-CuN) : DIN43710 Pt100 : IEC751(1995),JIS C1604-1997 JPt100 : JIS C1606-1989

CHINO CORPORATION


32-8 KUMANO-CHO, ITABASHI-KU, TOKYO 173-8632 Telephone : +81-3-3956-2171 Facsimile : +81-3-3956-0915 E-mail : inter@chino.co.jp Website : www.chino.co.jp/

DIMENSIONS

KR2000

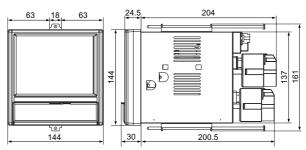

KR3000

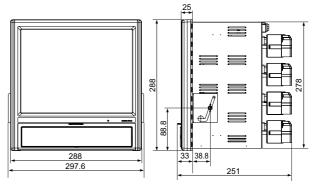

Unit: mm

AVAILABLE OPTIONS

Name	
Validation Document	
Traceability Certificate	
Installation Qualification (IQ) Certificate	
Operational Qualification (OQ) Certificate	

SOFTWARE (ZAILA-P) ENVIRONMENT

CPU	1GHz or faster
OS	Windows 2000/XP/Vista/7 *Internet Explorer 6.0 or later
Memory	256MB or more (512MB or more recommended)
Disk drive	CD-ROM drive: 1 drive or more Hard disk drive: Disk space of 1 drive or more for 100MB or more
Language	Japanese, English

Specifications subject to change without notice. Printed in Japan (I) 2011. 6